

# Schaller Genuine Spare Parts - Data Sheet

|                       |                                     |                    |                                           |
|-----------------------|-------------------------------------|--------------------|-------------------------------------------|
| <b>Material</b>       | <b>151481</b>                       | <b>Description</b> | <b>Spare Part Kit 1 (Maintenance Kit)</b> |
| <b>Applicable for</b> | <b>VISATRON VN87 &amp; VN87plus</b> |                    |                                           |


## 1) Maintenance Schedule

| Step | Description                                     | Intervall (whatever comes first) |       |       |       |        |        |        |        | See Section  | Required Parts / Tools |
|------|-------------------------------------------------|----------------------------------|-------|-------|-------|--------|--------|--------|--------|--------------|------------------------|
|      | Hours,                                          | 2.000                            | 4.000 | 6.000 | 8.000 | 10.000 | 12.000 | 14.000 | 16.000 |              |                        |
|      | or Months                                       | 3                                | 6     | 9     | 12    | 15     | 18     | 21     | 24     |              |                        |
| 4    | Exchange air filters in Measuring Head          | X                                | X     | X     | X     | X      | X      | X      | X      | 5.3, Page 42 | 151481 Maintenance Kit |
| 6    | Exchange air filters in Pressure Regulator Unit |                                  | X     |       | X     |        | X      |        | X      | 5.4, Page 42 | 151481 Maintenance Kit |

## 2) Maintenance kit content

| Material | Material (old) | Description                                               | Qty | Unit | Item Line    |
|----------|----------------|-----------------------------------------------------------|-----|------|--------------|
| 365197   | 10042          | Sinter brass 22x2, Filter Disc                            | 10  | PC   | Position: 3  |
| 365198   | 10041          | Circlip D22 DIN472                                        | 4   | PC   | Position: 32 |
| 365206   | 10002          | Filter for Pressure Reducer                               | 3   | PC   | Position: 10 |
| 365208   | 10003          | O-Ring 9,0x4,5 NBR70 screw Pres. Reducer                  | 3   | PC   | Position: 19 |
| 355636   | 11070          | Gasket for Inspection cover VN87 <sup>plus</sup>          | 2   | PC   | Position: 70 |
| 366717   | -              | Filter cartridge (blue for new pressure regulator 273440) | 2   | PC   |              |

Note: Quantity sufficient for 1 year / 8.000 hours as for Steps 4 + 6 of Maintenance Schedule (plus spare)

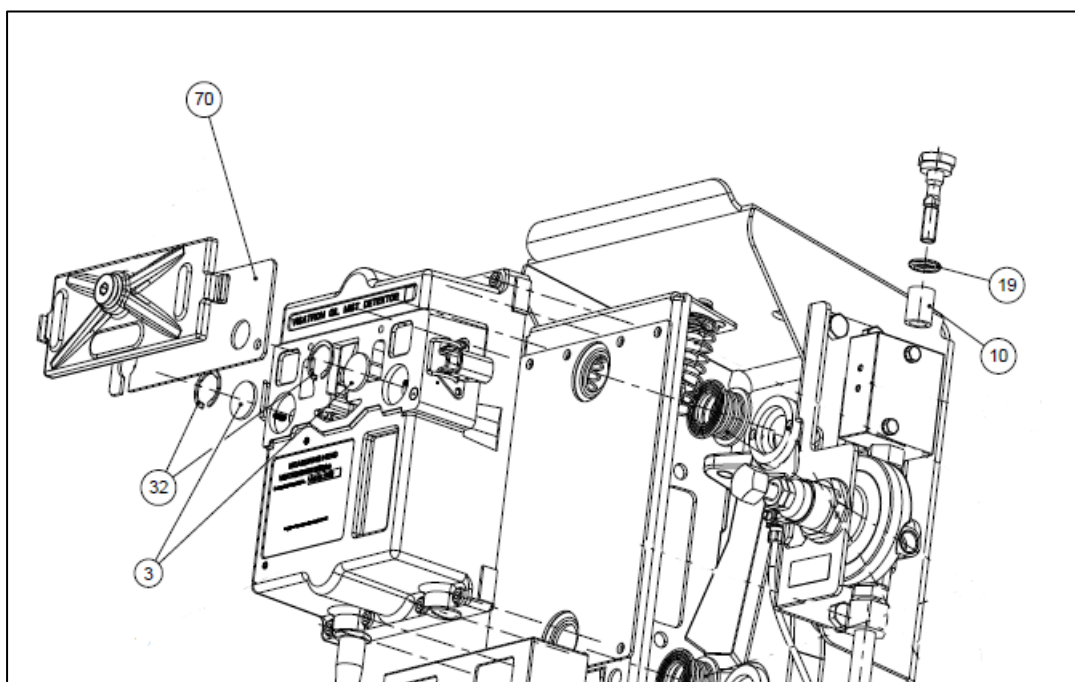

## Schaller Genuine Spare Parts - Data Sheet

|                |                          |             |                                    |
|----------------|--------------------------|-------------|------------------------------------|
| Material       | 151481                   | Description | Spare Part Kit 1 (Maintenance Kit) |
| Applicable for | VISATRON VN87 & VN87plus |             |                                    |

